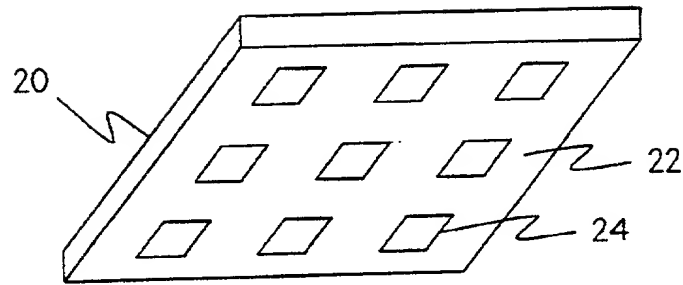
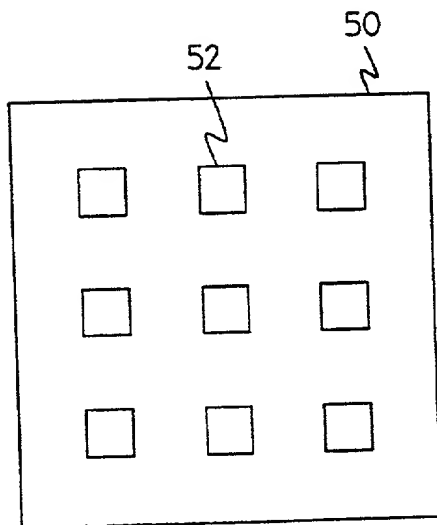


094466-04701




CALIBRATION  
RETICLE

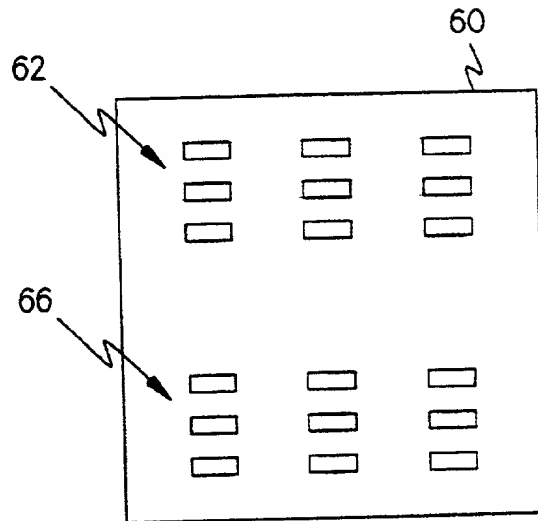Fig- 1B1



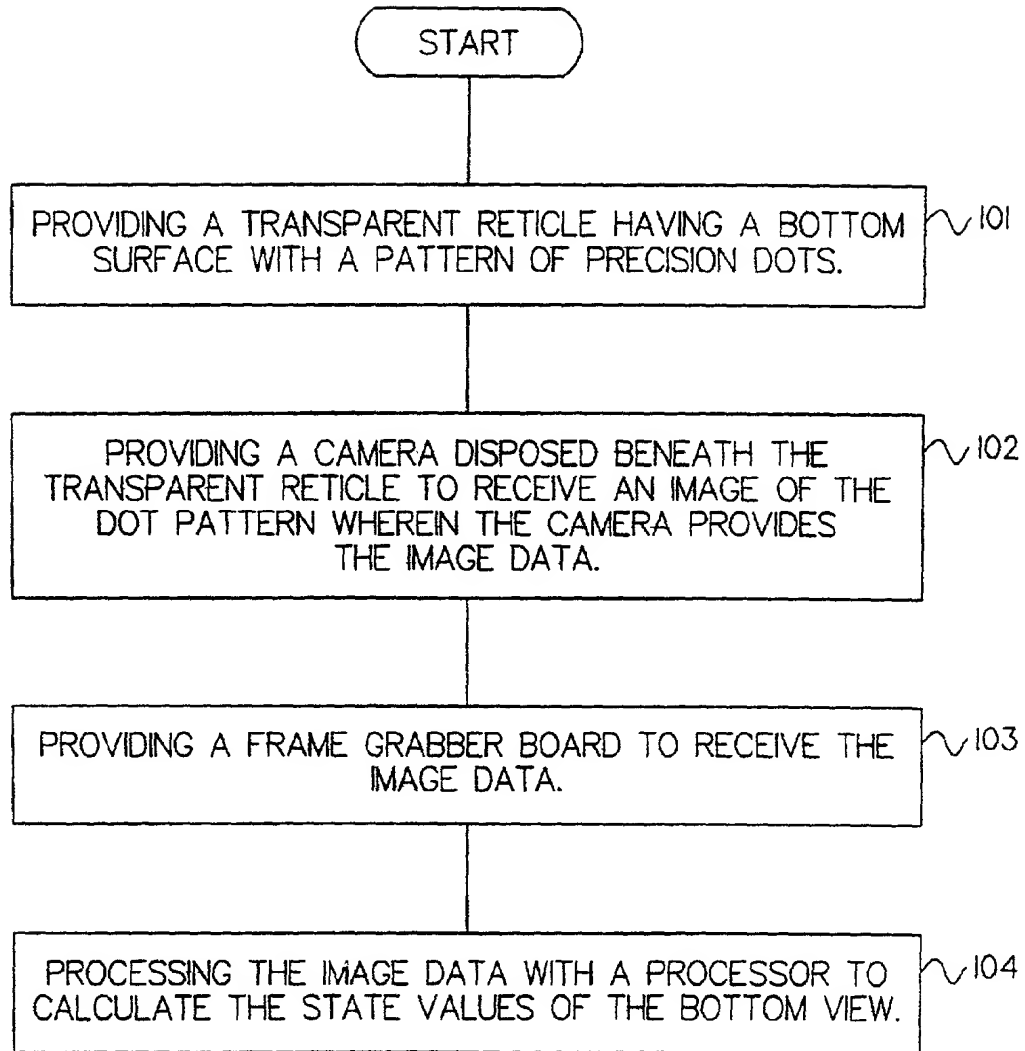
BOTTOM VIEW  
IMAGE

Fig- 1B2



2 SIDE VIEWS  
IMAGE

Fig- 1B3

Fig. 2A


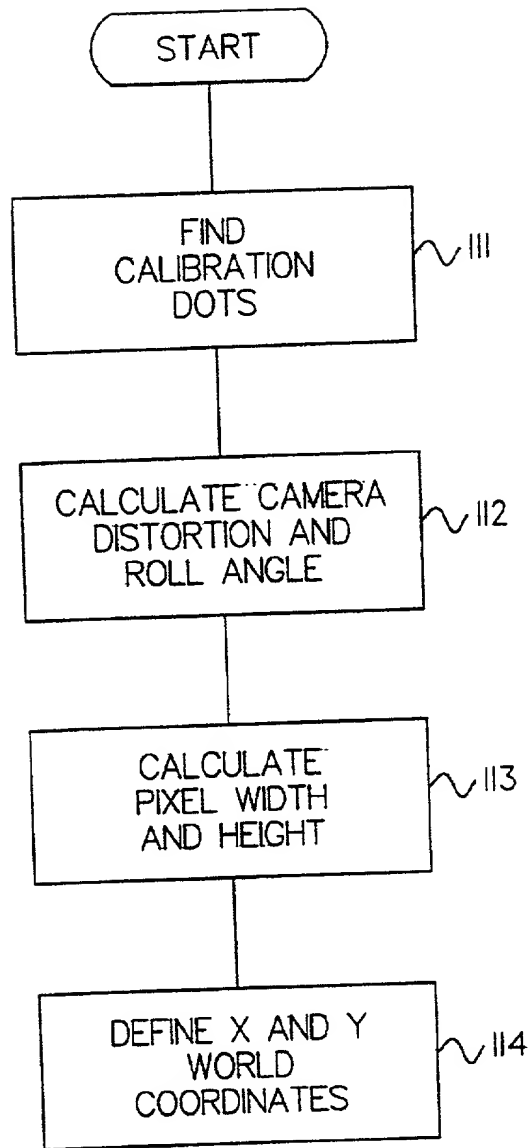
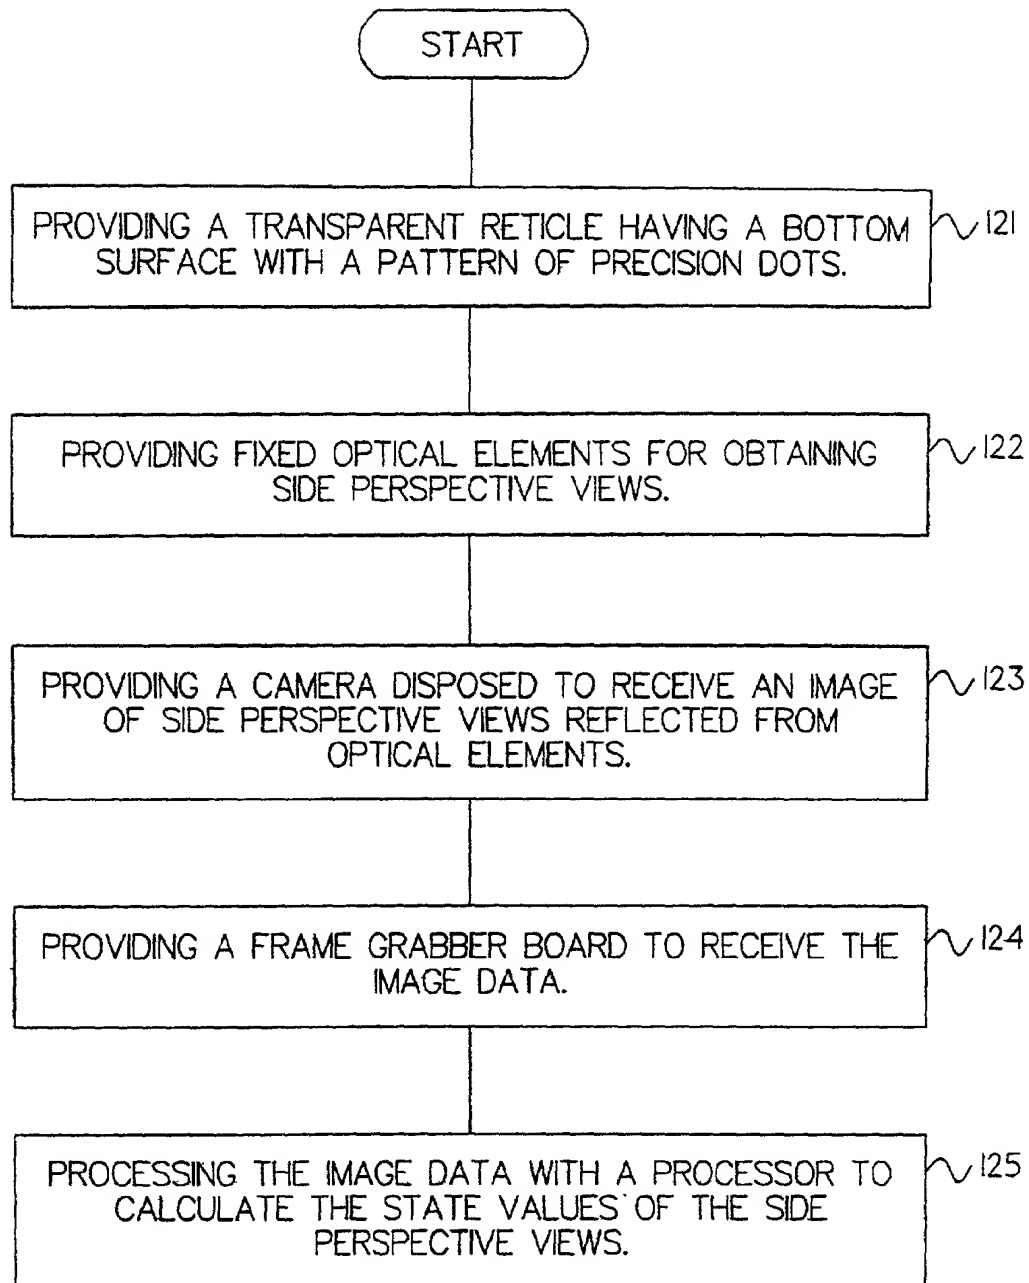


Fig- 2B

0944626-042701

Fig-2C

Fig- 2D

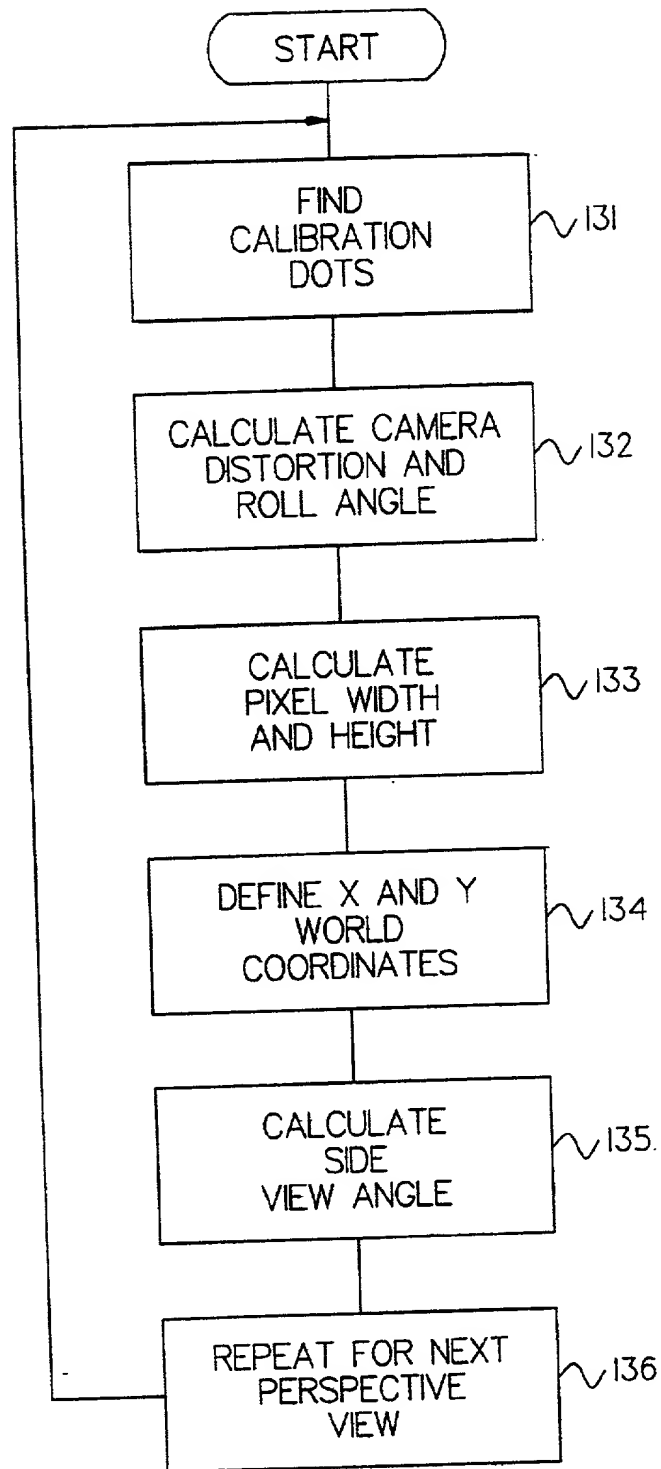


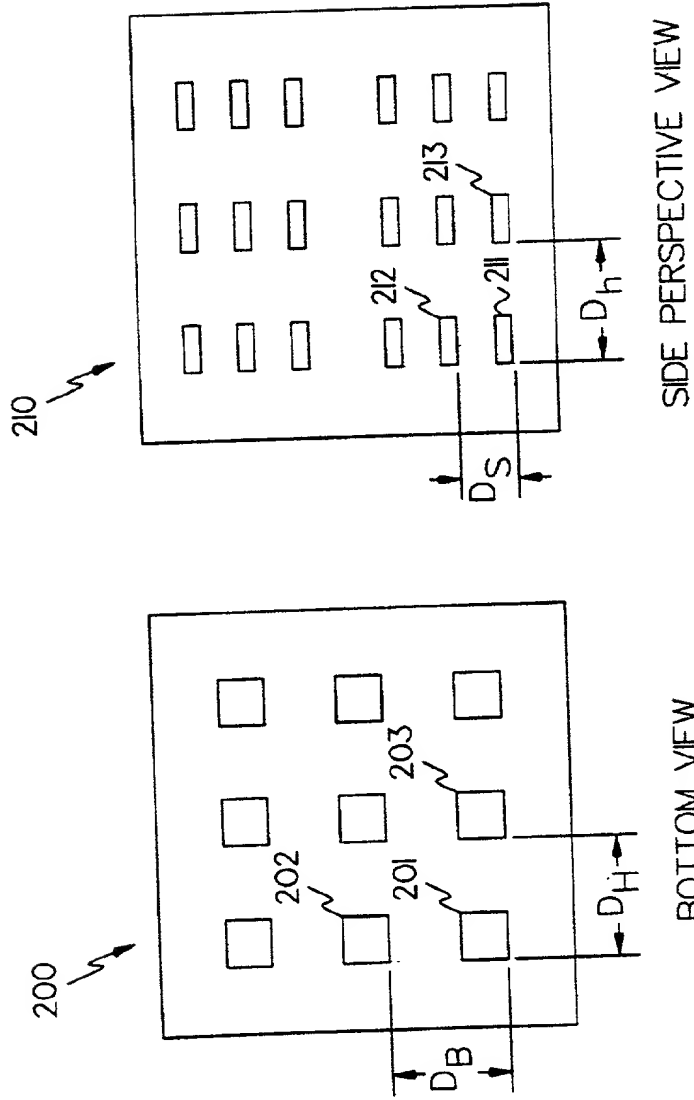


FIG-2F2

FIG-2F1

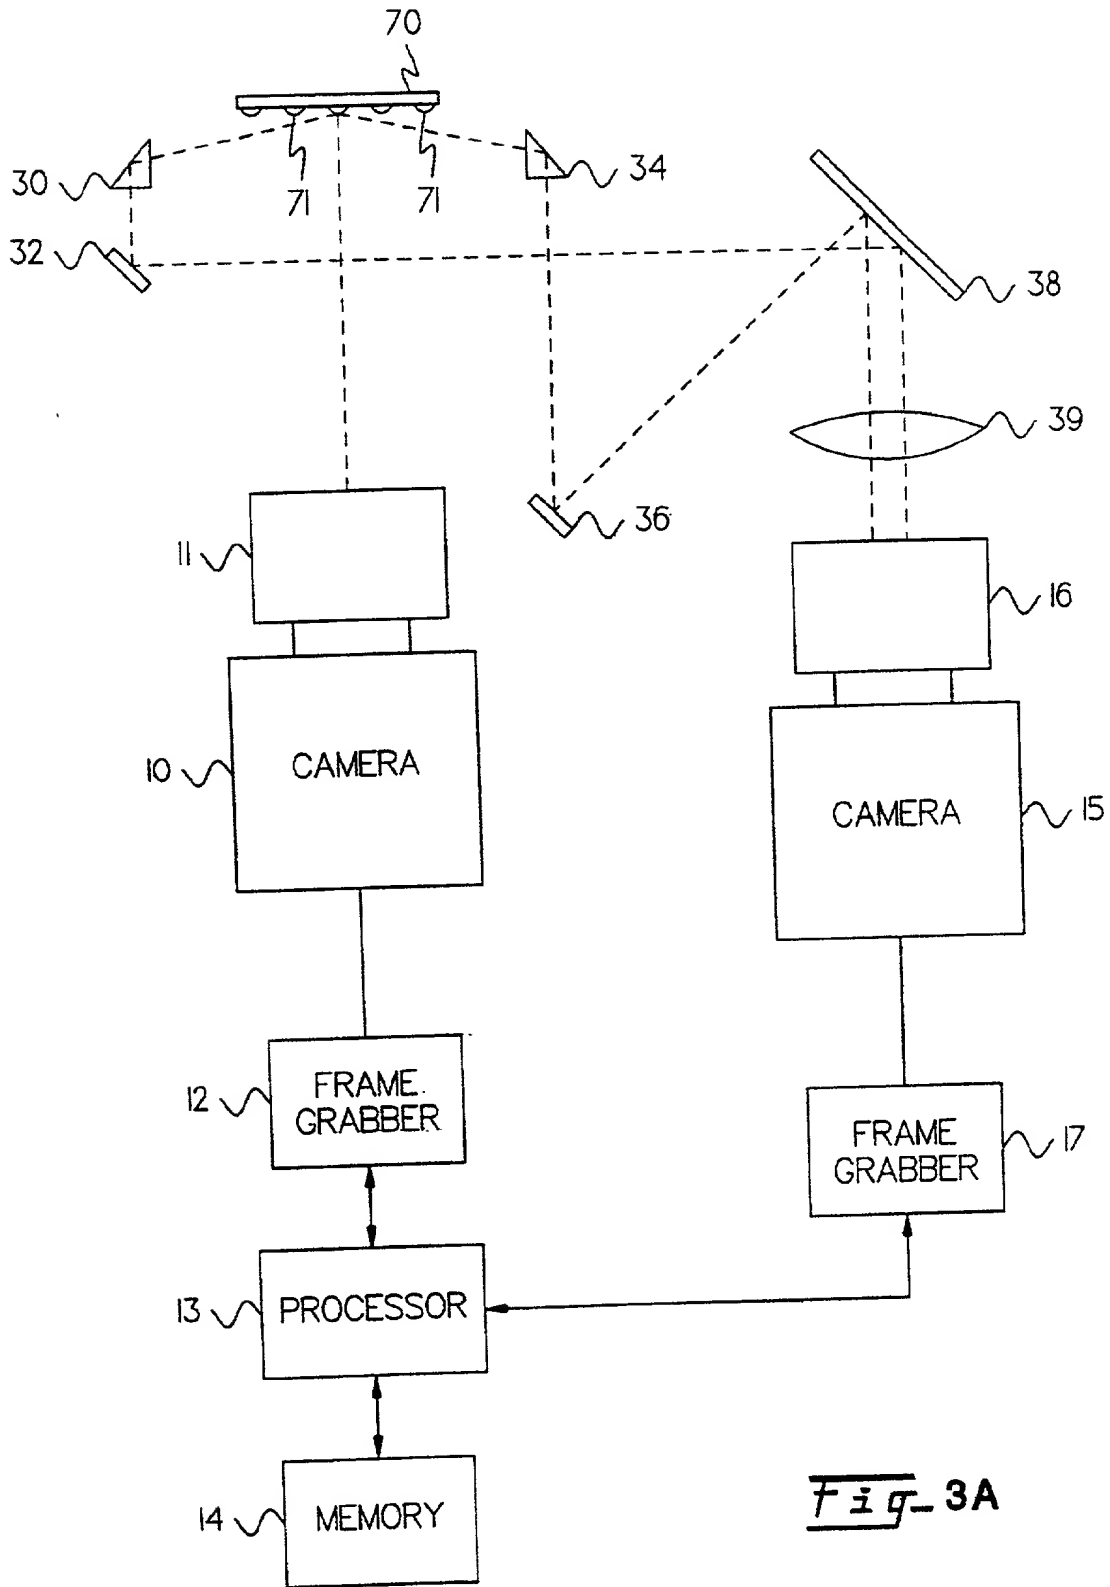




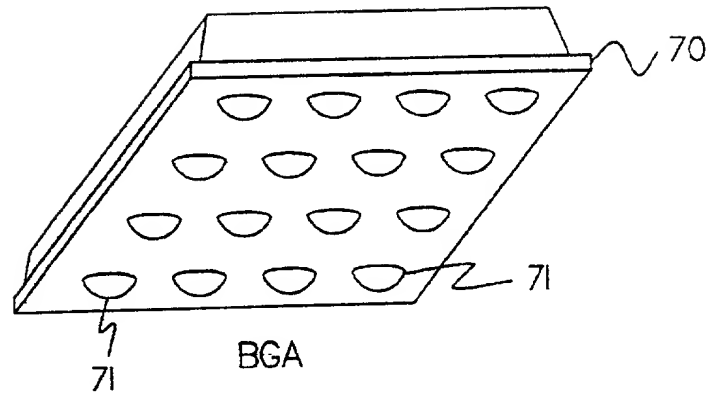
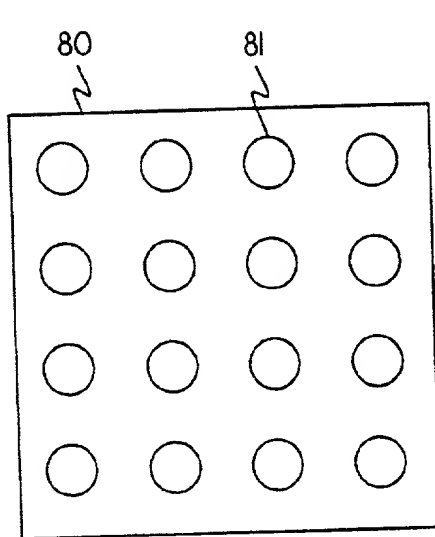


Fig- 3B1

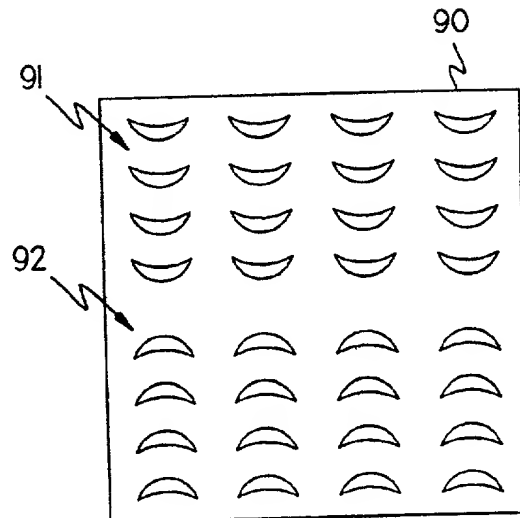

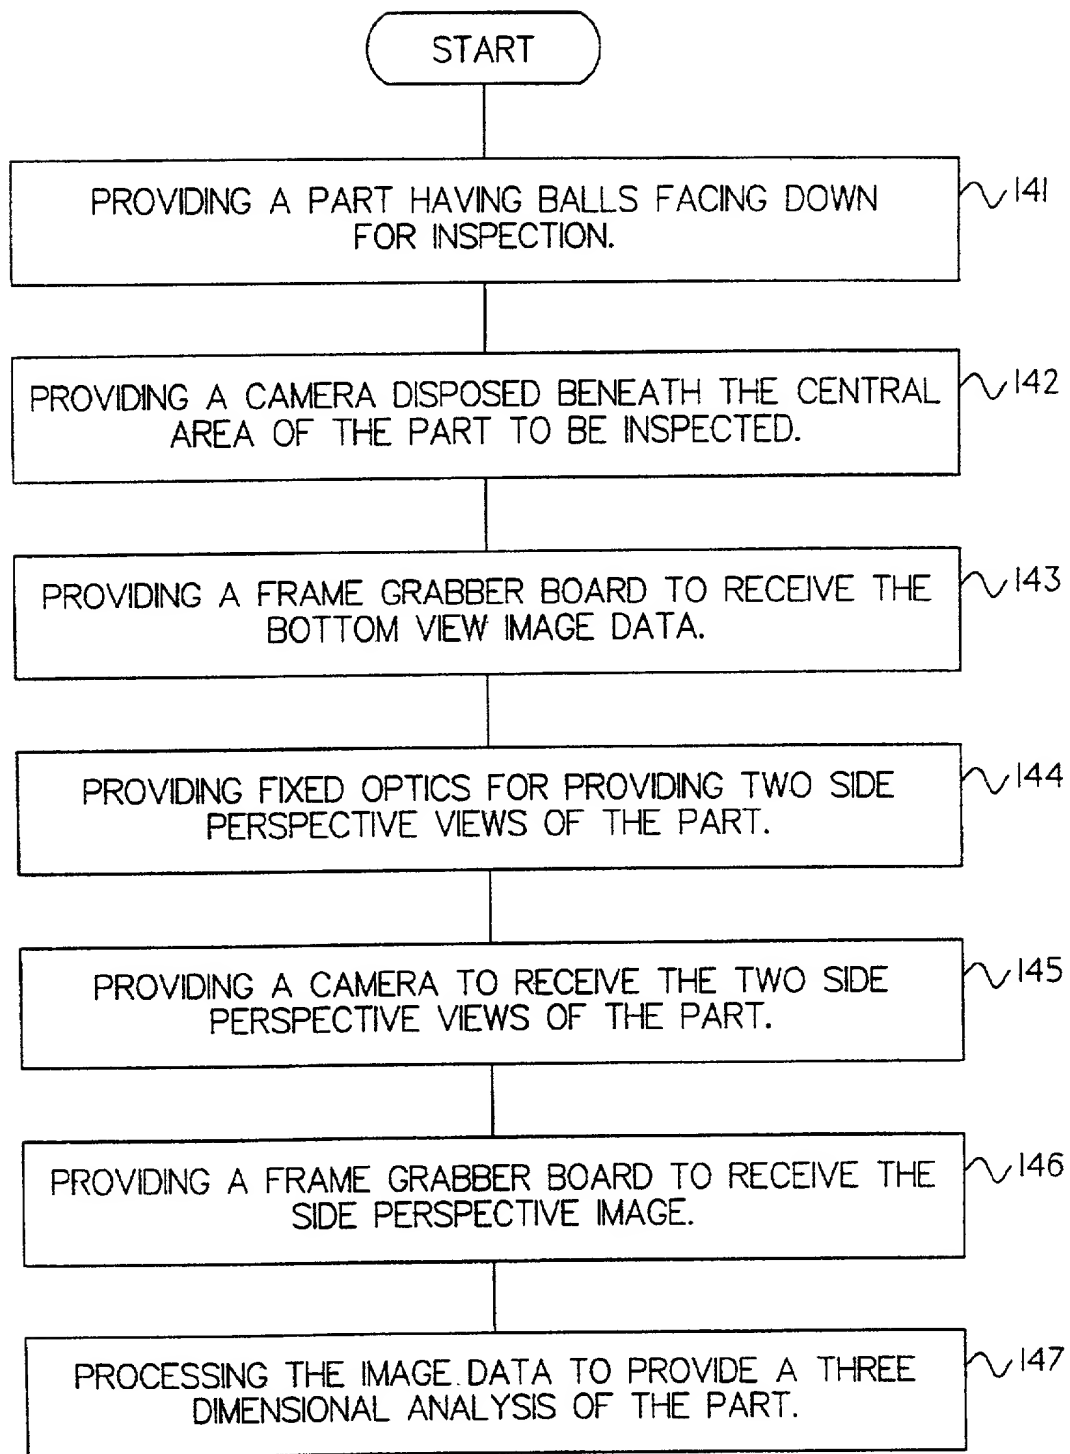
BOTTOM VIEW  
IMAGE

Fig- 3B2



2 SIDE VIEWS  
IMAGE

Fig- 3B3

Fig-4

12/30

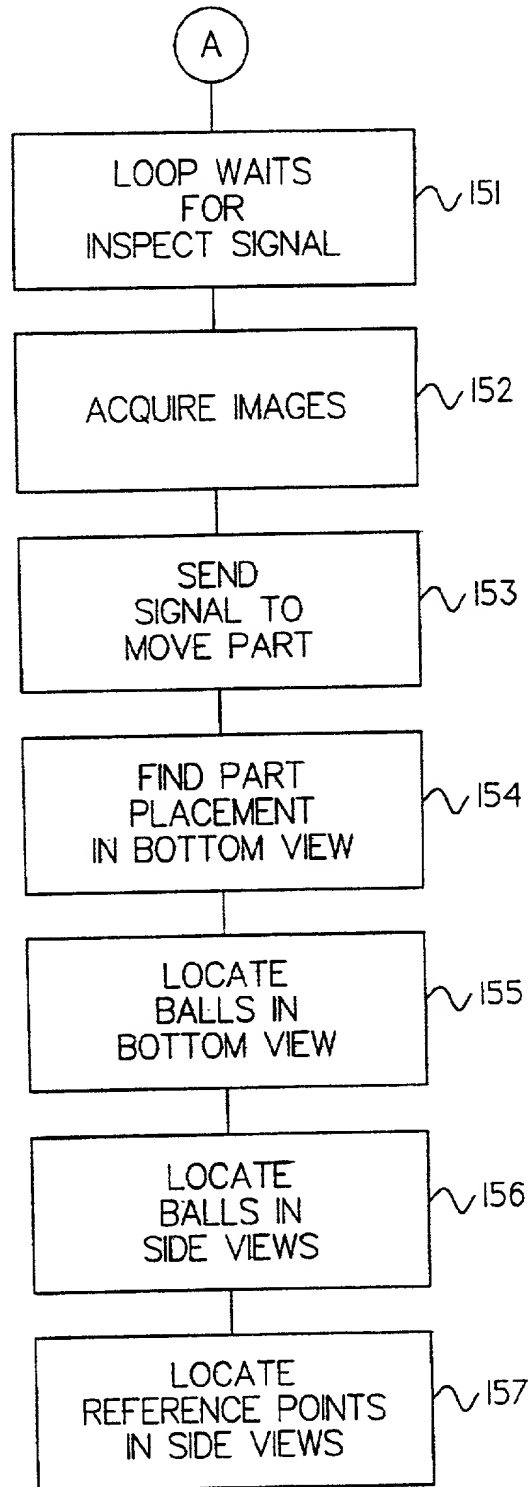


Fig- 5A


Fig- 5B



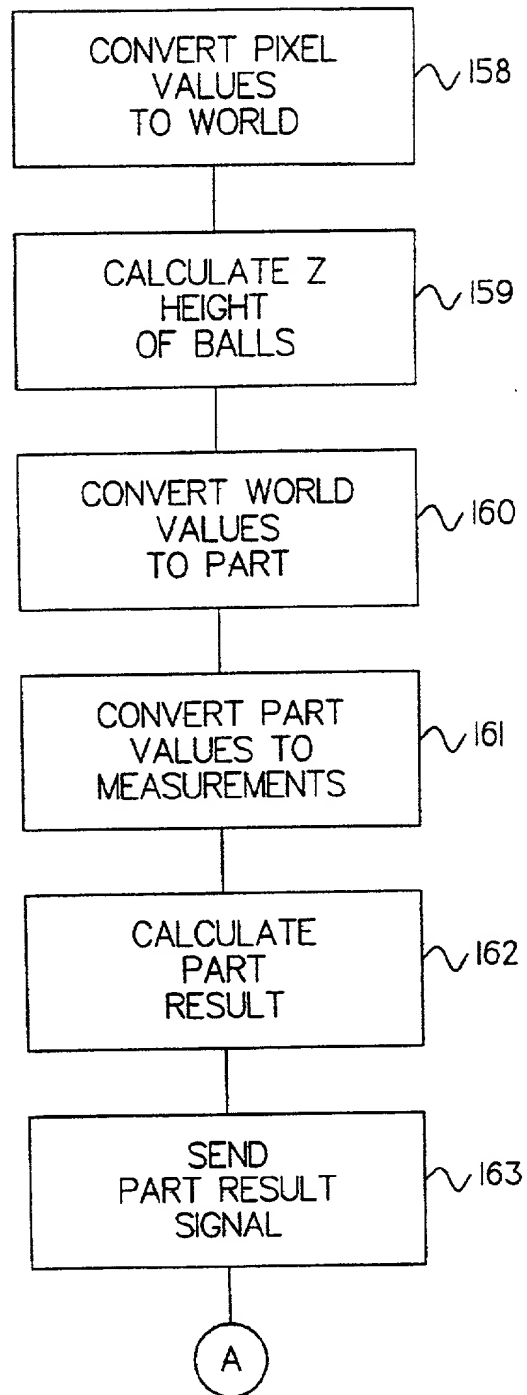FIG. 2A-D: 9234-4850




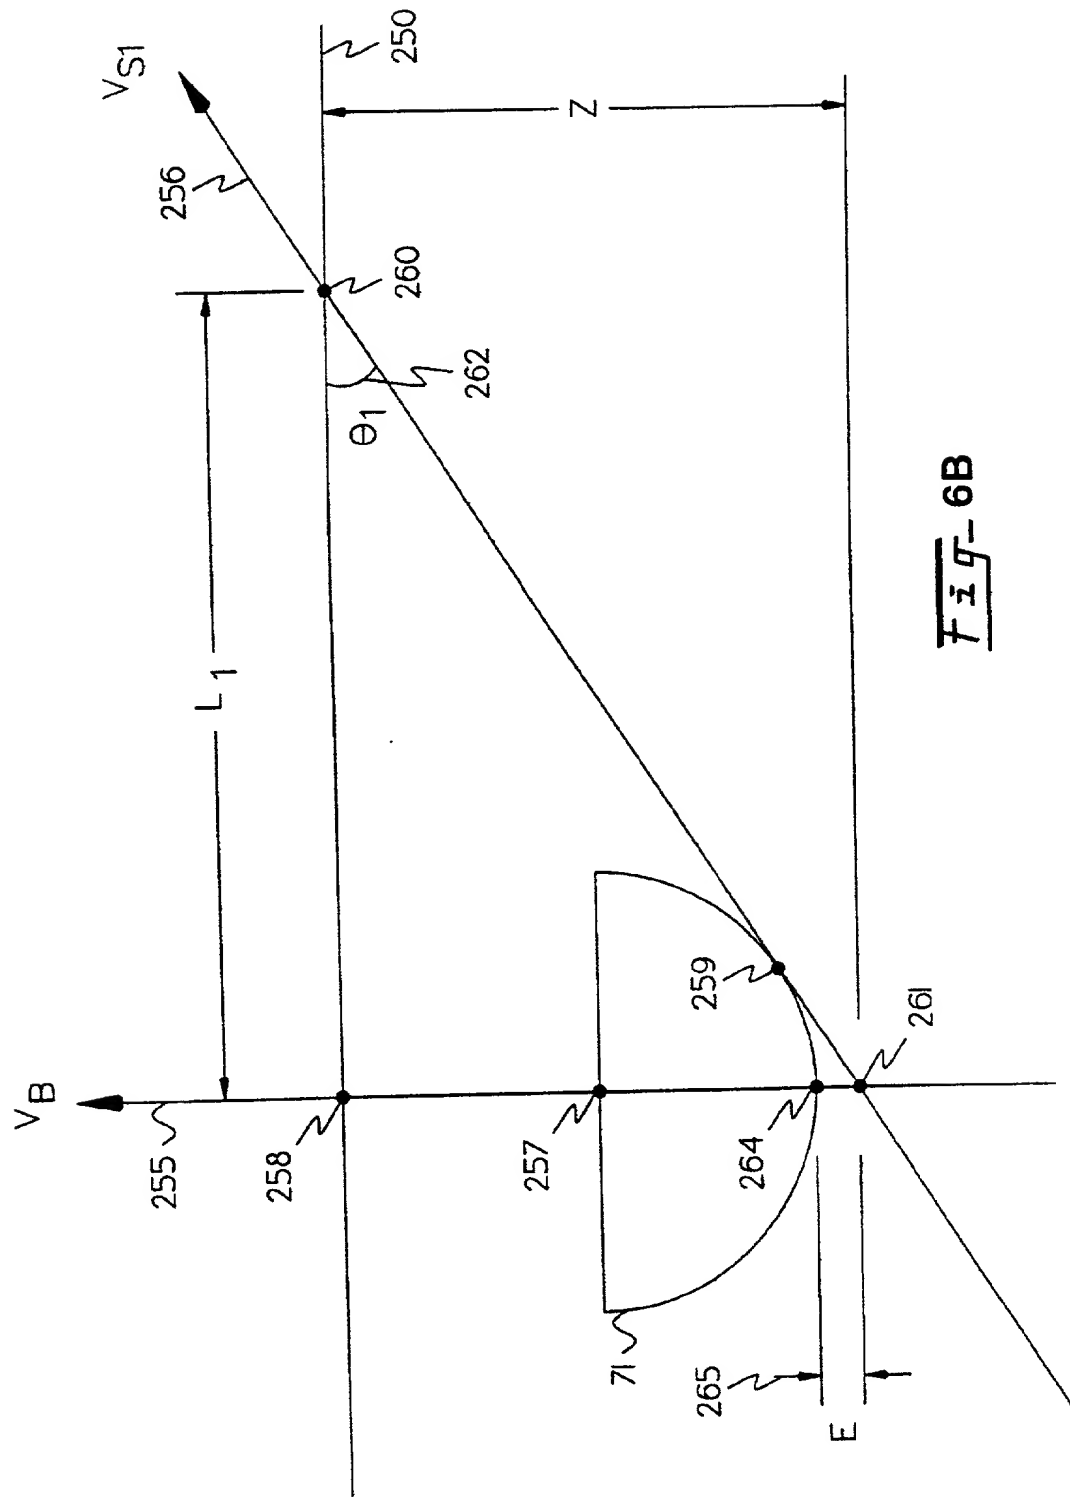


FIG. 2A-D

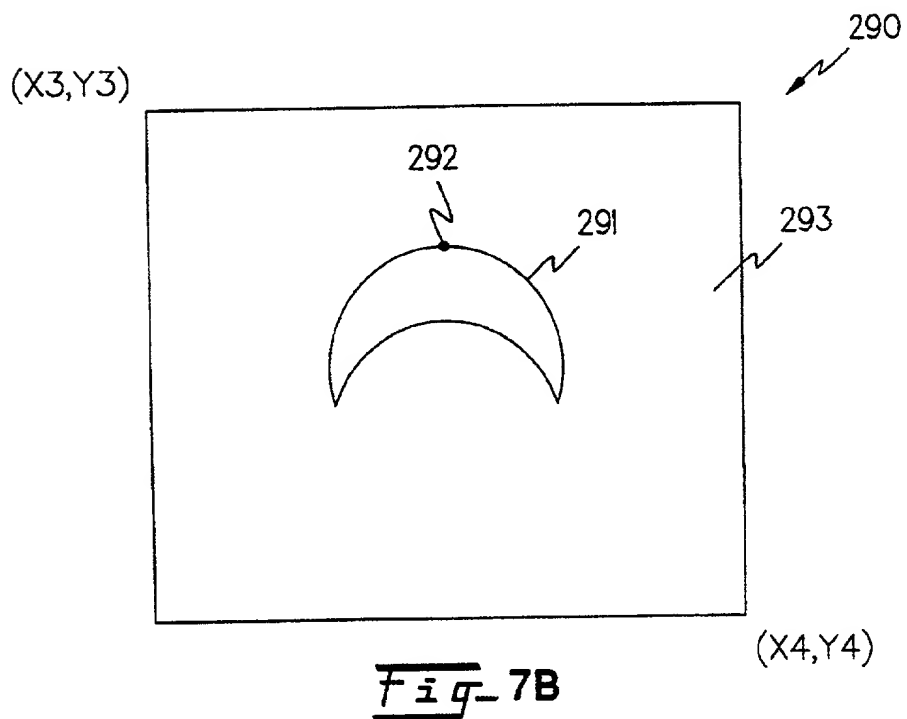


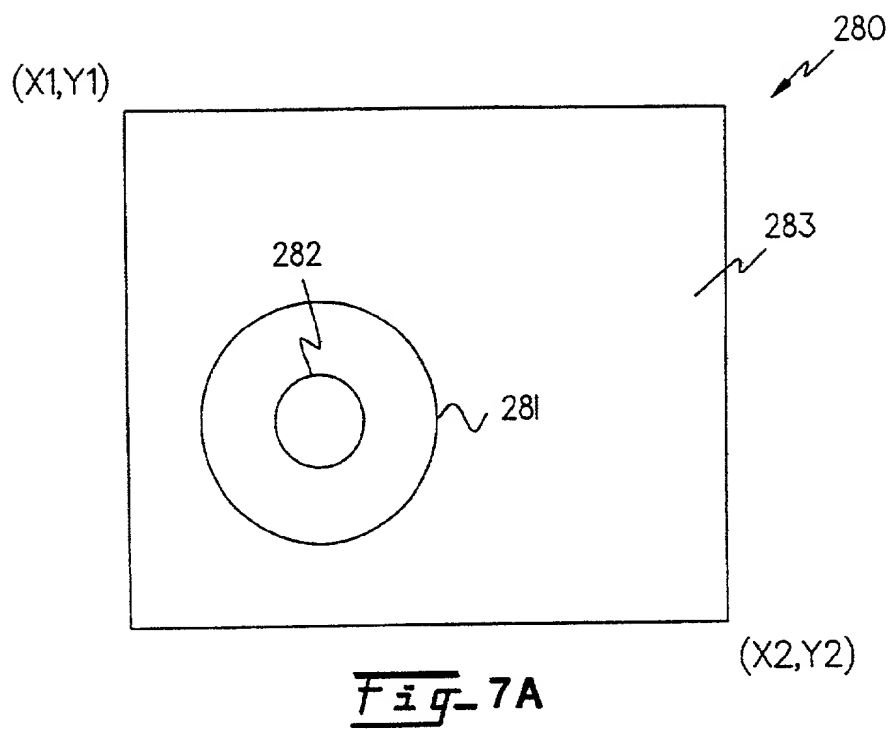

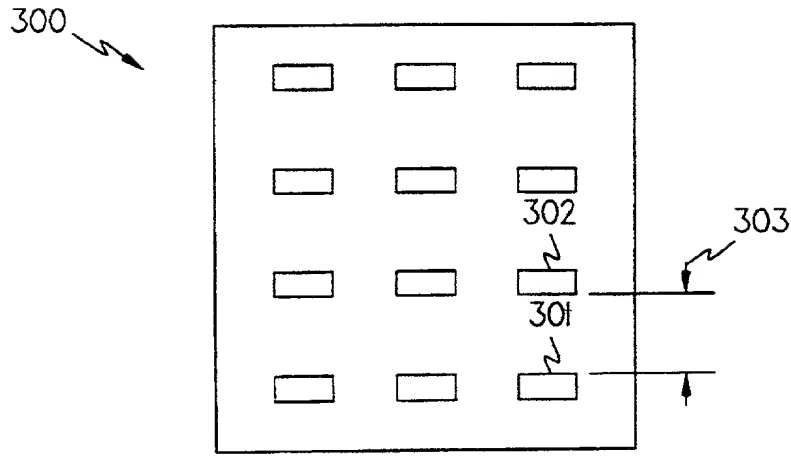

2 SIDE VIEWS  
CALIBRATION PATTERN

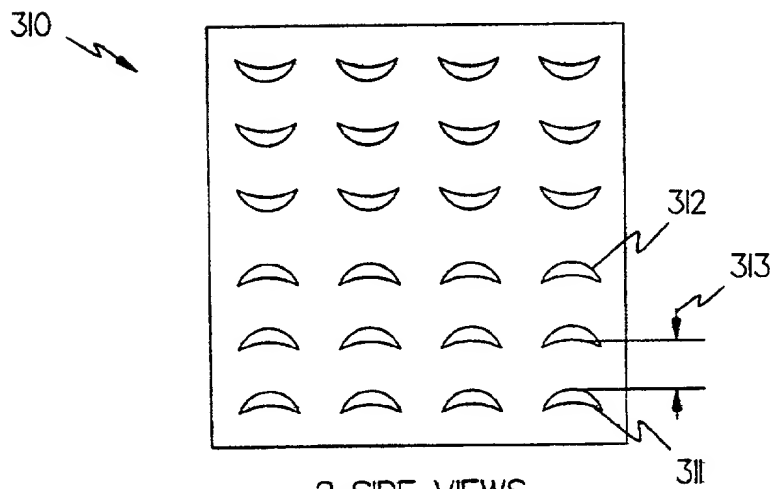Fig- 8A




2 SIDE VIEWS  
BALLS

Fig- 8B

Downloaded from www.gettyimages.com

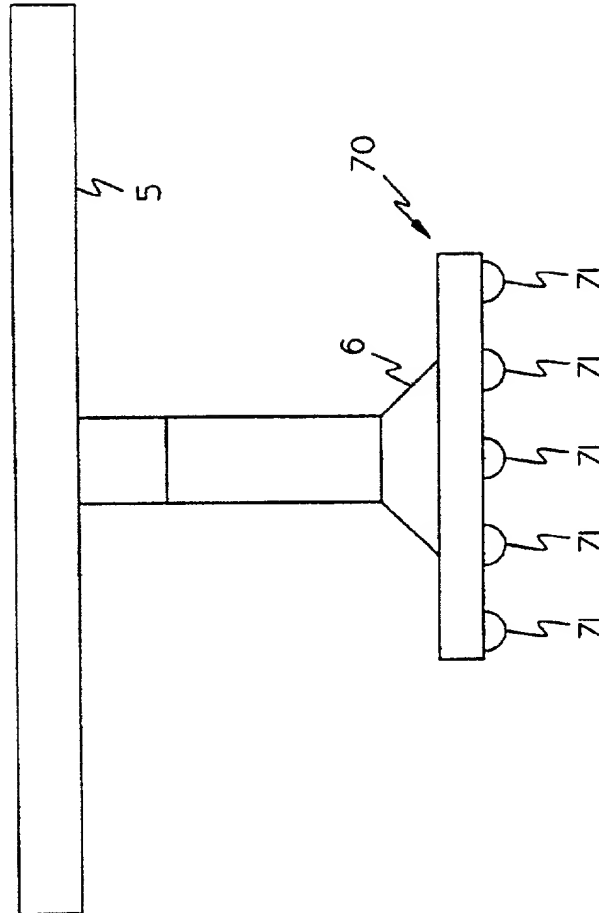Fig-9




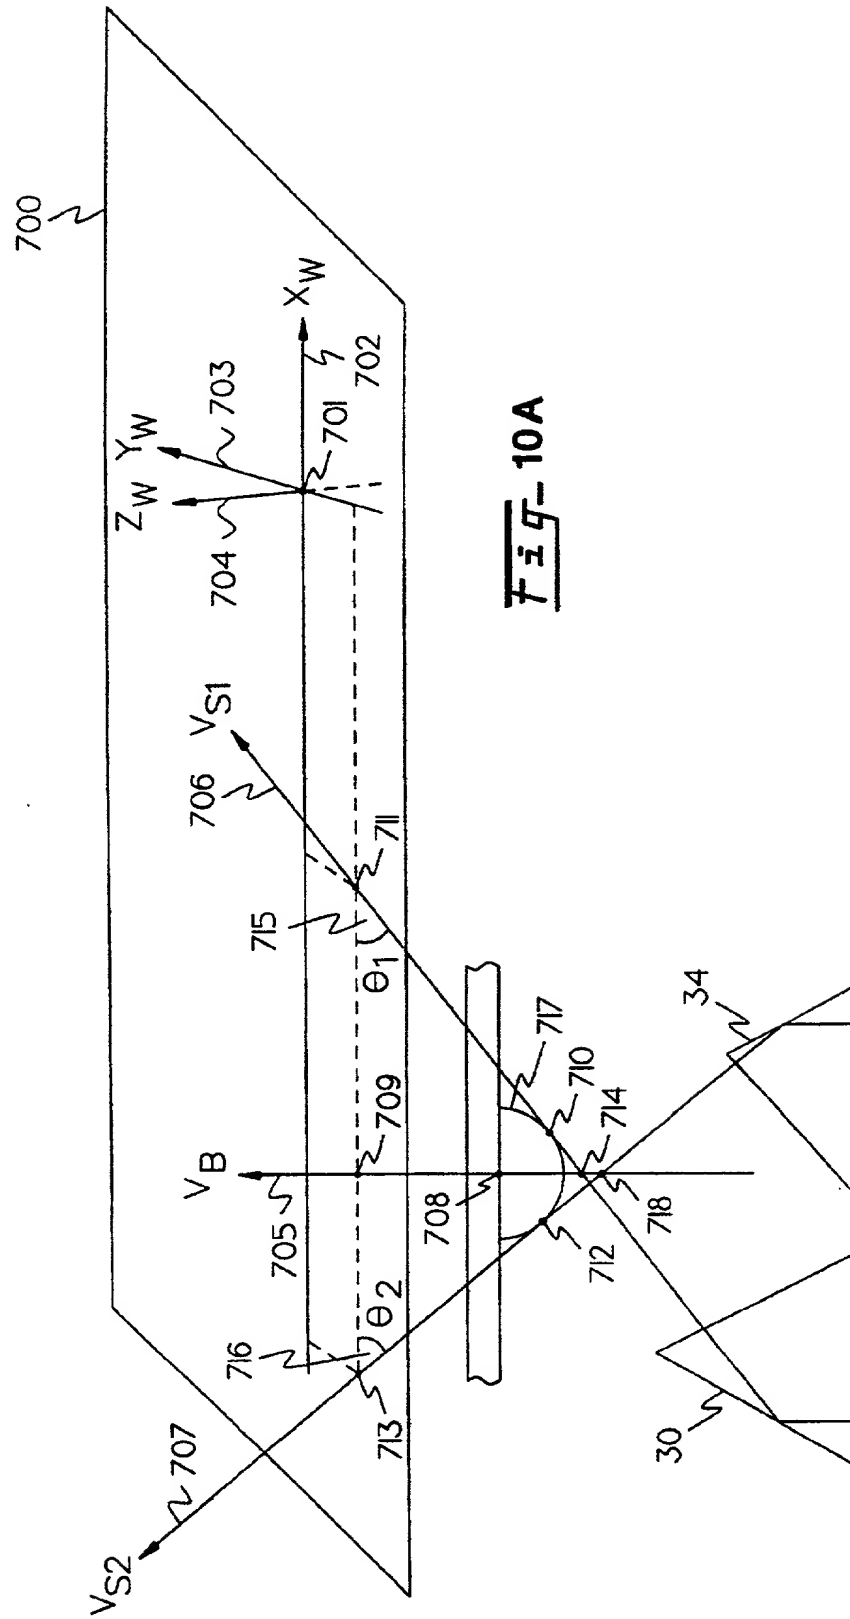
[illegible]

Table 1. Demographic characteristics of the study population	
Age (years)	50.0 ± 10.0
Gender	
Male	50 (50.0%)
Female	50 (50.0%)
Education (years)	12.0 ± 2.0
Marital status	
Married	40 (80.0%)
Single	10 (20.0%)
Occupation	
Professional	20 (40.0%)
Managerial	10 (20.0%)
Technical	10 (20.0%)
Service	10 (20.0%)
Unemployed	10 (20.0%)
Health status	
Good	40 (80.0%)
Fair	10 (20.0%)
Poor	0 (0.0%)
Smoking status	
Smoker	10 (20.0%)
Non-smoker	40 (80.0%)
Alcohol consumption	
Regular	10 (20.0%)
Occasional	10 (20.0%)
Never	30 (60.0%)
Exercise frequency	
Regular	10 (20.0%)
Occasional	10 (20.0%)
Never	30 (60.0%)
Stress level	
High	10 (20.0%)
Medium	10 (20.0%)
Low	30 (60.0%)
Family size	3.0 ± 1.0
Income (USD/month)	1500 ± 500
Health insurance	
Yes	40 (80.0%)
No	10 (20.0%)
Comorbidities	
Hypertension	10 (20.0%)
Diabetes	5 (10.0%)
Cholesterol	10 (20.0%)
Asthma	5 (10.0%)
Depression	10 (20.0%)
Other	5 (10.0%)
Medication use	
Regular	10 (20.0%)
Occasional	10 (20.0%)
Never	30 (60.0%)
Healthcare utilization	
Regular	10 (20.0%)
Occasional	10 (20.0%)
Never	30 (60.0%)
Healthcare satisfaction	
Satisfied	30 (60.0%)
Dissatisfied	20 (40.0%)
Healthcare access	
Easy	30 (60.0%)
Difficult	20 (40.0%)
Healthcare cost	
Low	30 (60.0%)
High	20 (40.0%)
Healthcare quality	
Good	30 (60.0%)
Fair	10 (20.0%)
Poor	10 (20.0%)
Healthcare safety	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare effectiveness	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare equity	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare sustainability	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare innovation	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare leadership	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare governance	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare accountability	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare transparency	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare integrity	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare ethics	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare justice	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare solidarity	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare cooperation	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare partnership	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare collaboration	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare communication	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare information	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare knowledge	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare skills	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare attitudes	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (20.0%)
Healthcare beliefs	
High	30 (60.0%)
Medium	10 (20.0%)
Low	10 (2

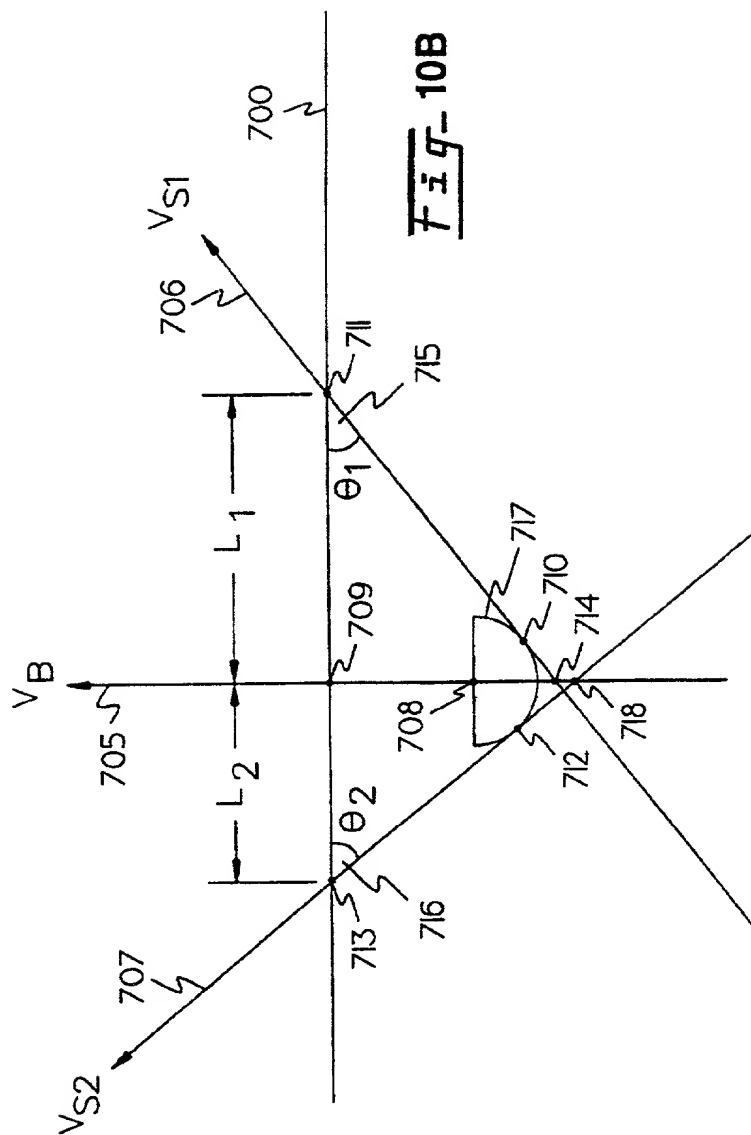



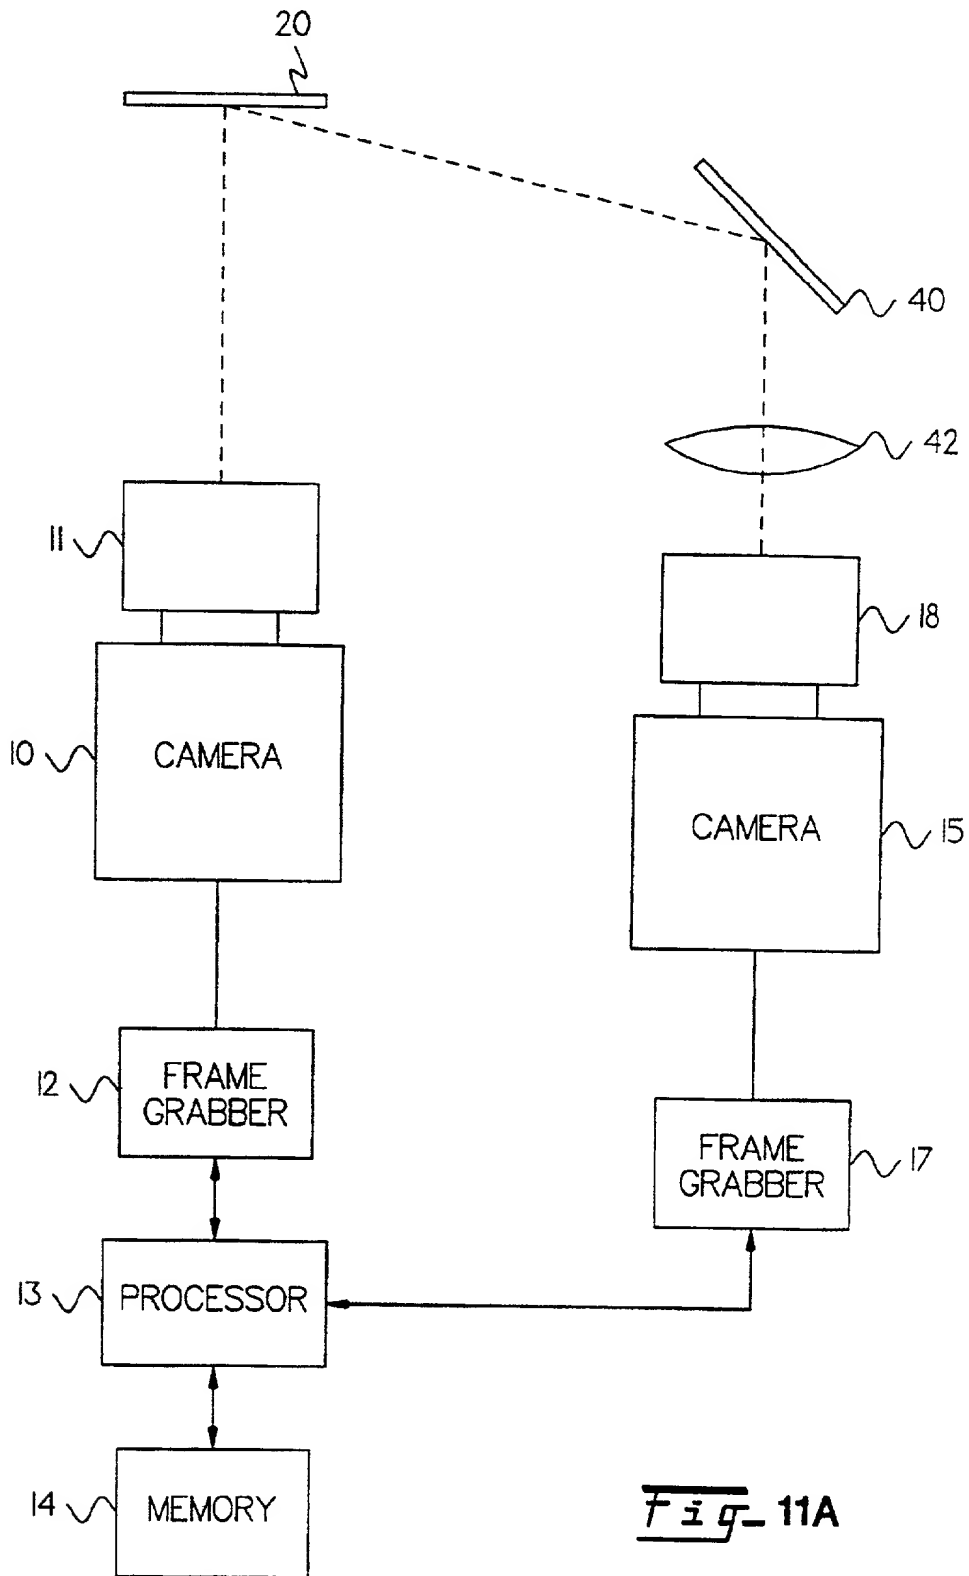


Fig. 11A

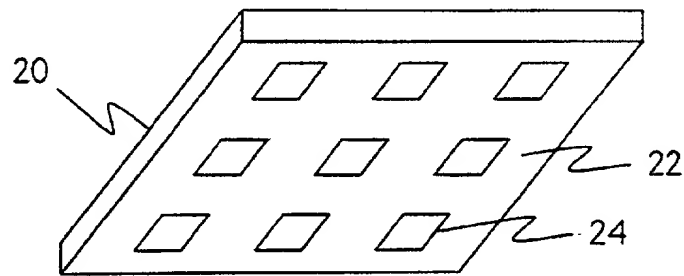


CALIBRATION  
RETICLE

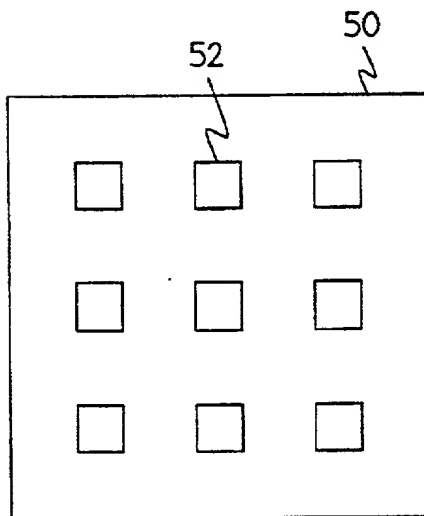Fig- 11B1



BOTTOM VIEW IMAGE

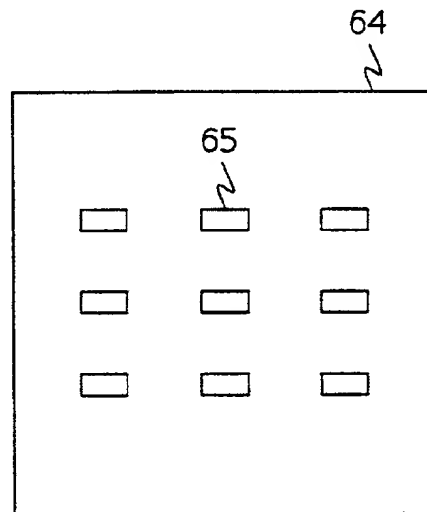Fig- 11B2



SIDE VIEW IMAGE

Fig- 11B3

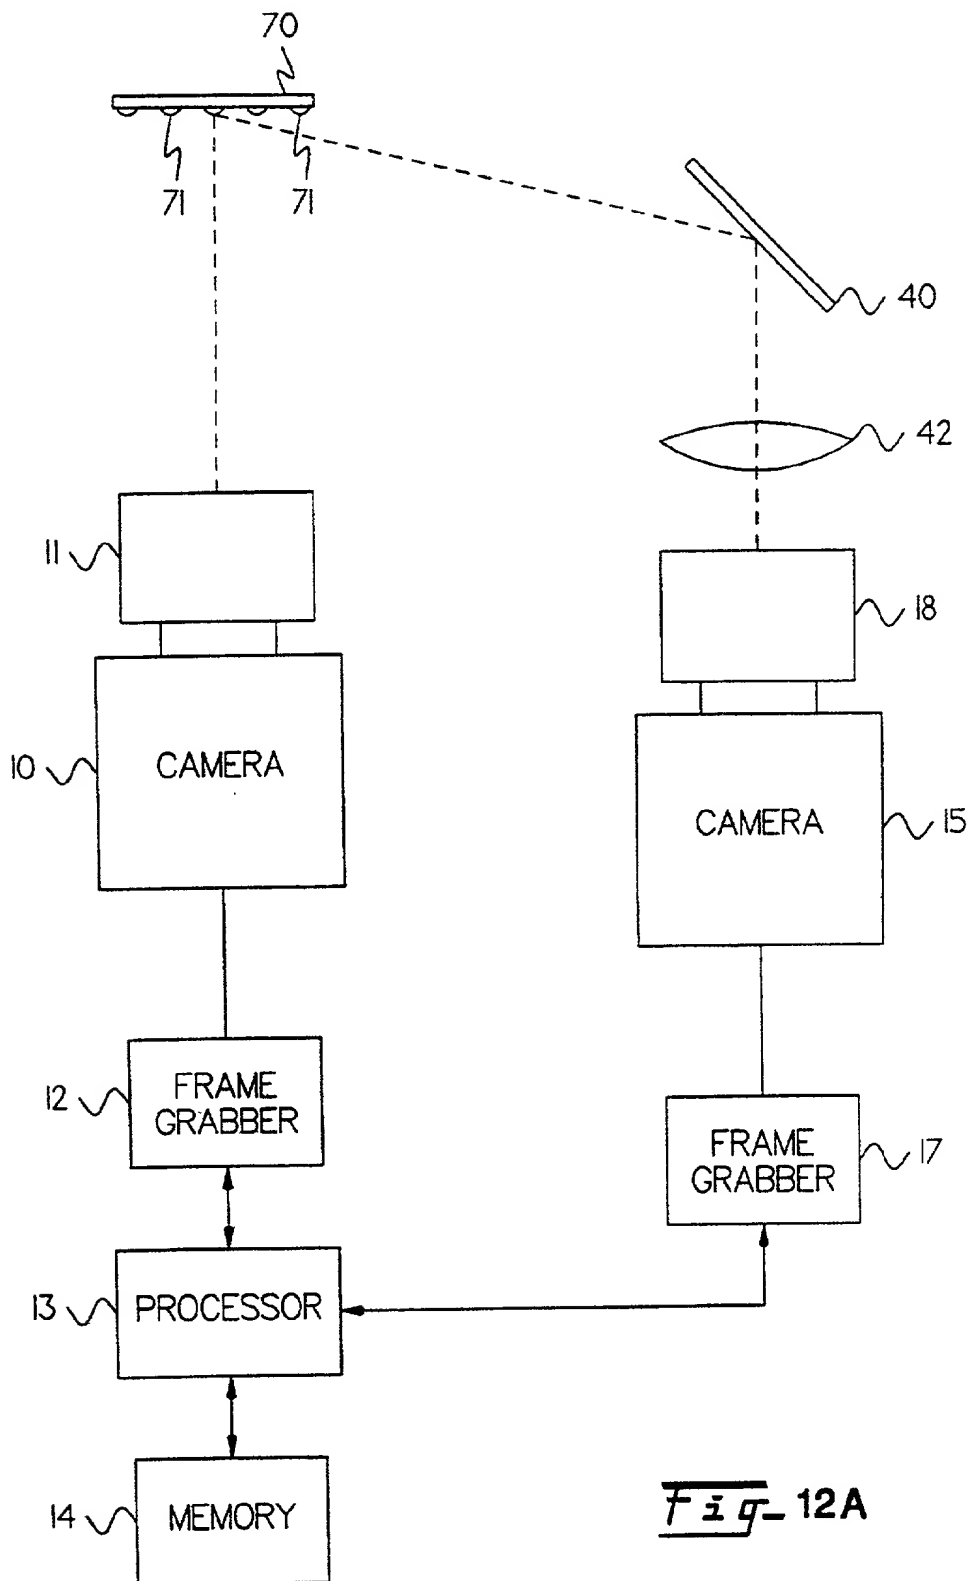


Fig- 12A

09344526-04701



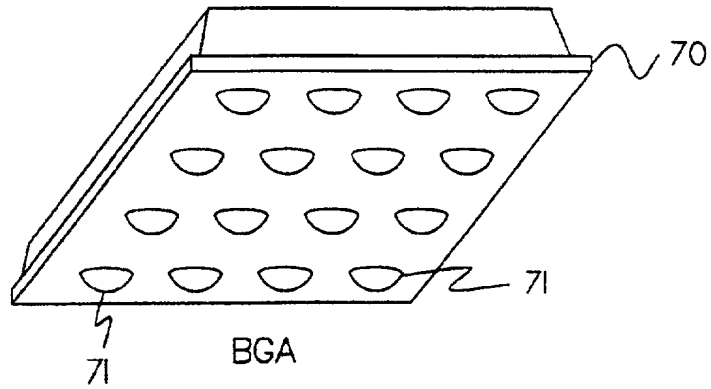


Fig. 12B1

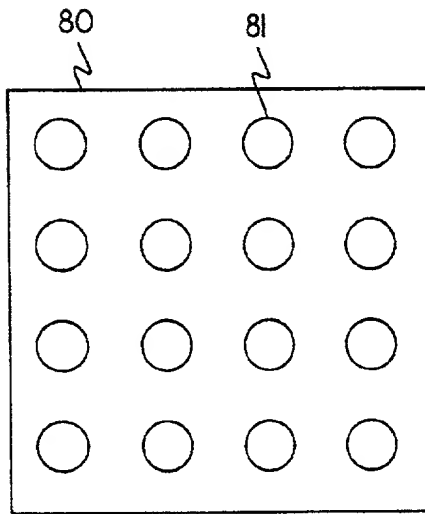

BOTTOM VIEW IMAGE

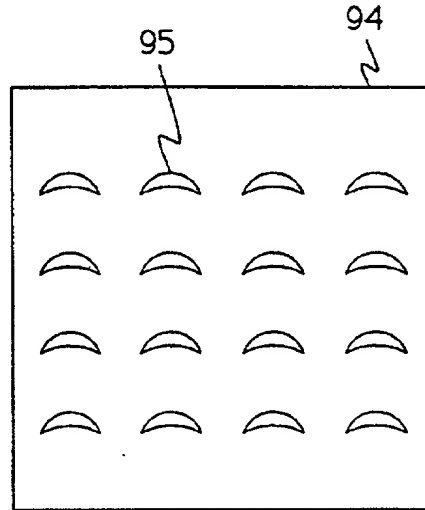Fig. 12B2




SIDE VIEW IMAGE


Fig. 12B3



Fig. 13

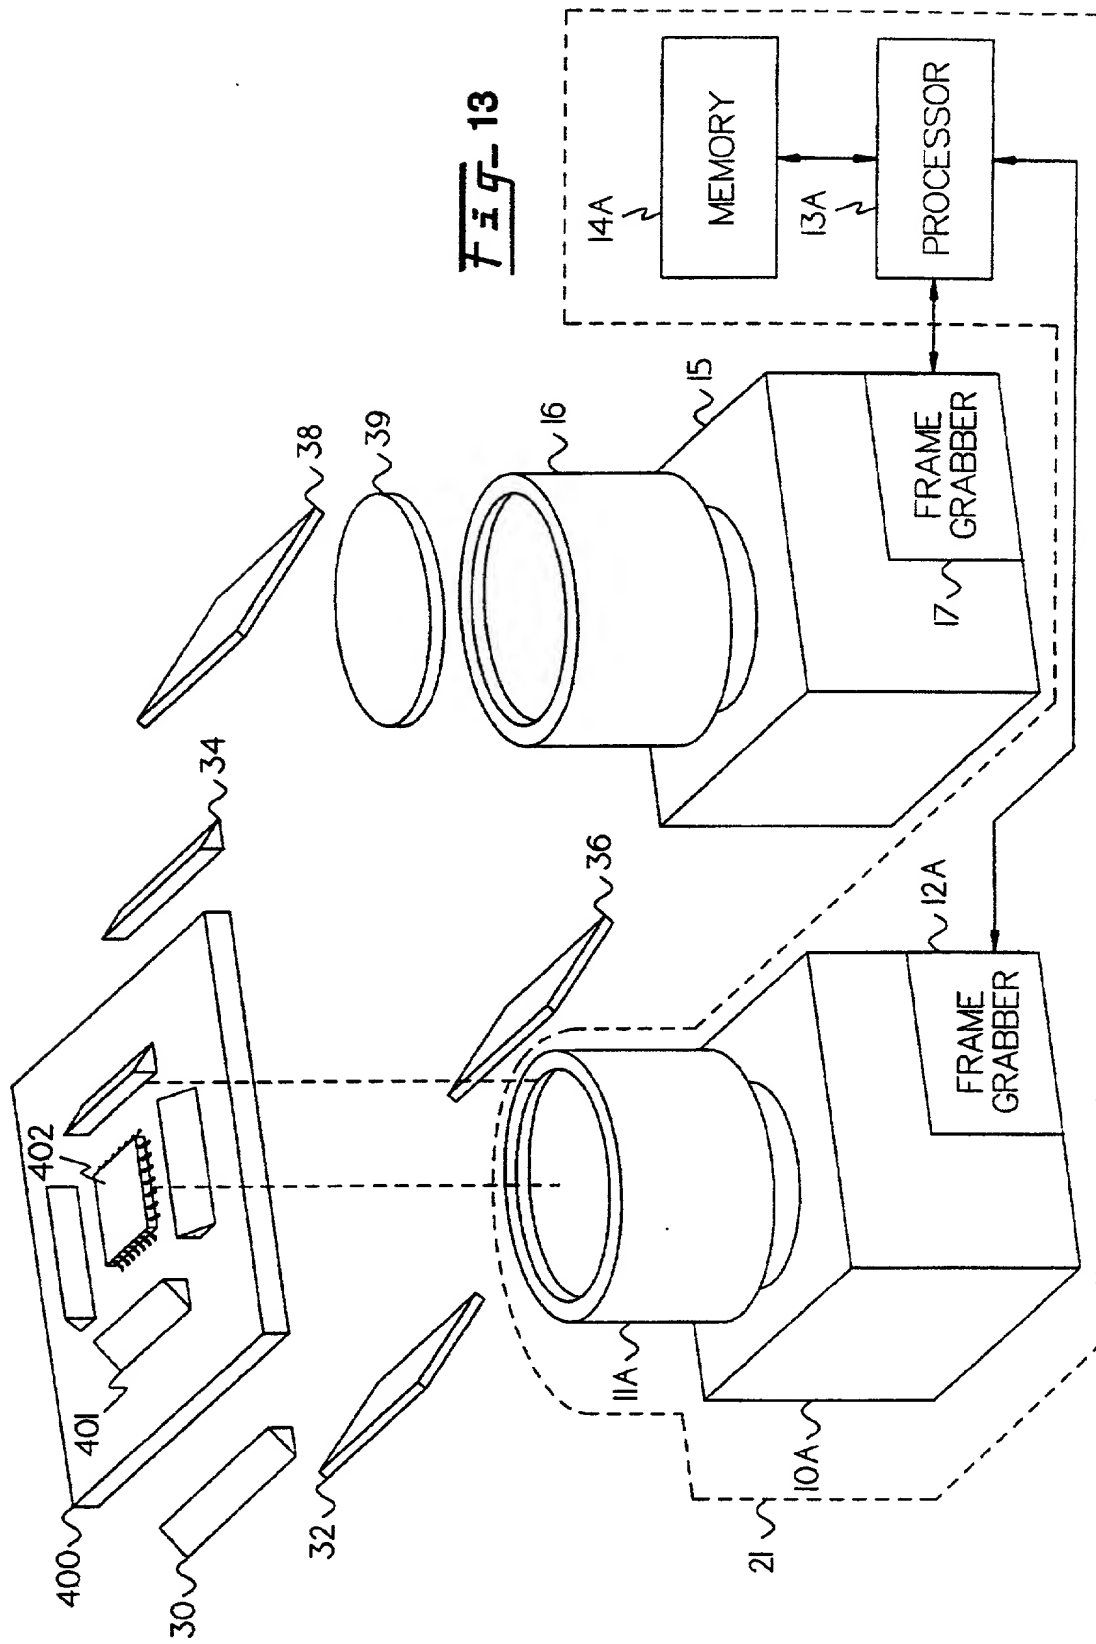

**Fig- 14**

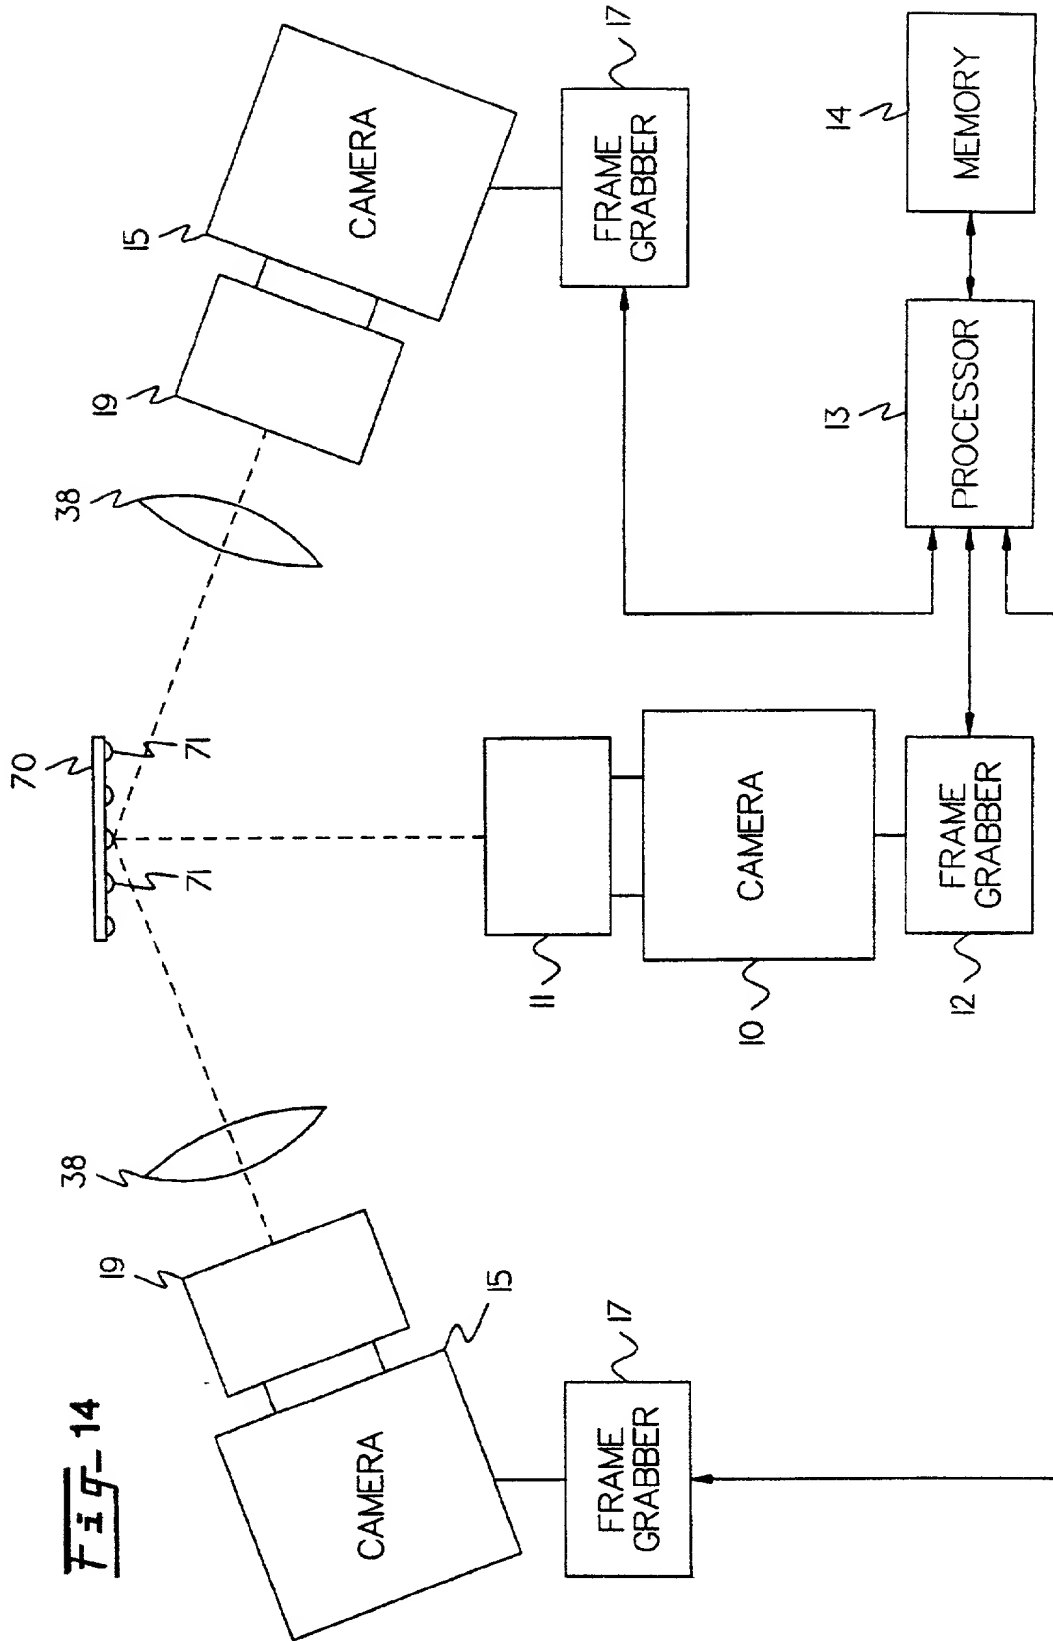


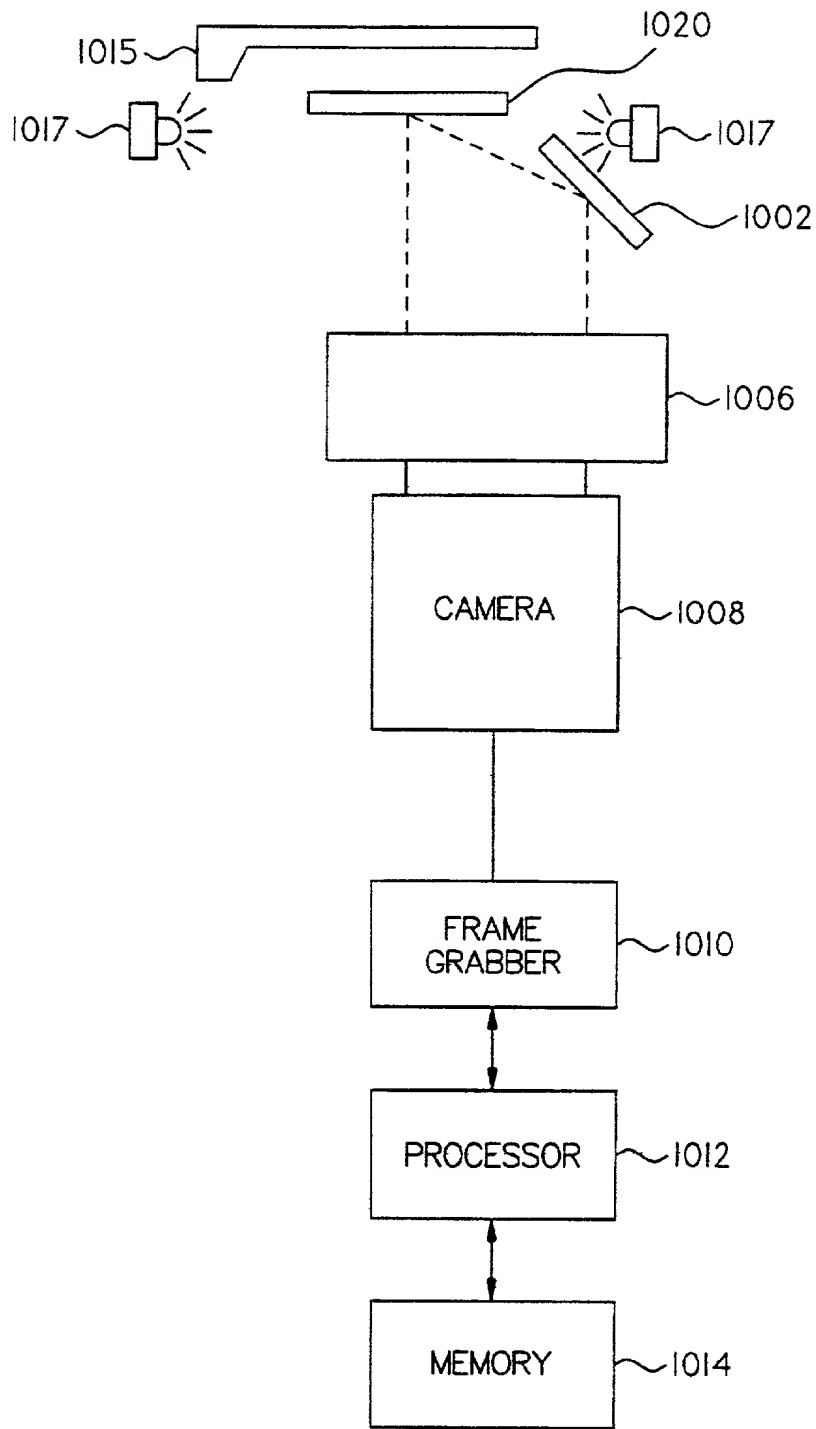



Fig. 15

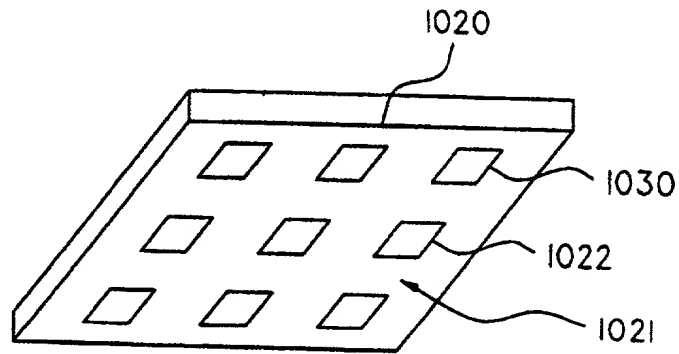0934456-042701



CALIBRATION  
RETICLE

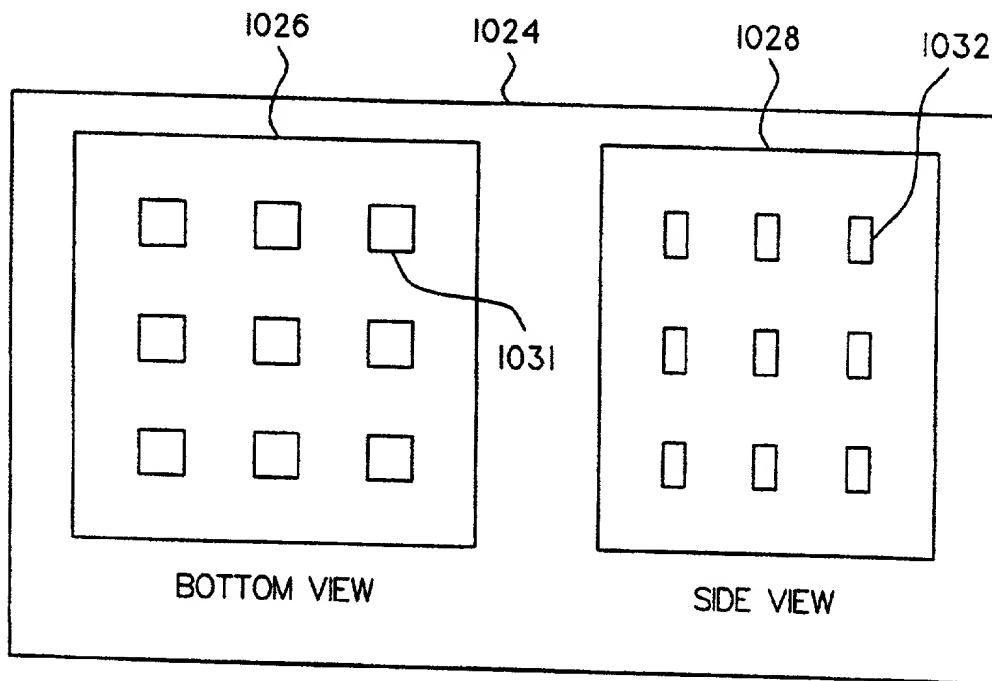Fig. 16A



BOTTOM VIEW

SIDE VIEW

IMAGE

Fig. 16B

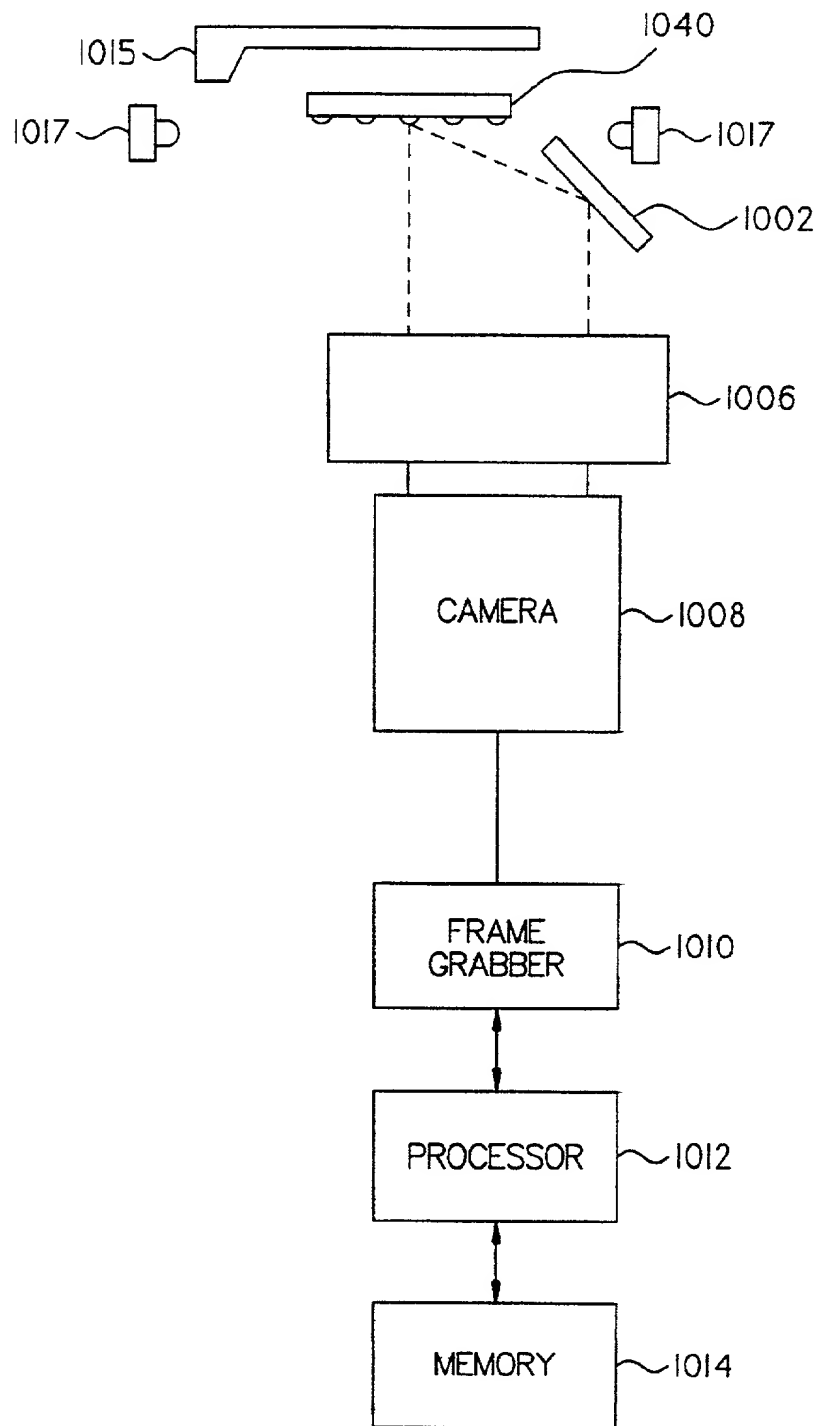


Fig-17

09344629-04201

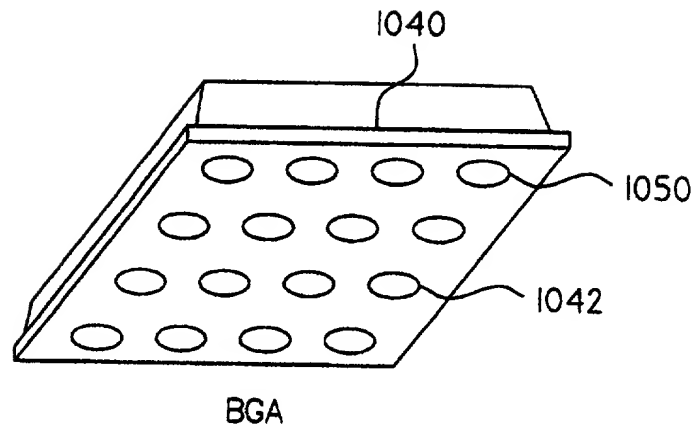


Fig. 18A

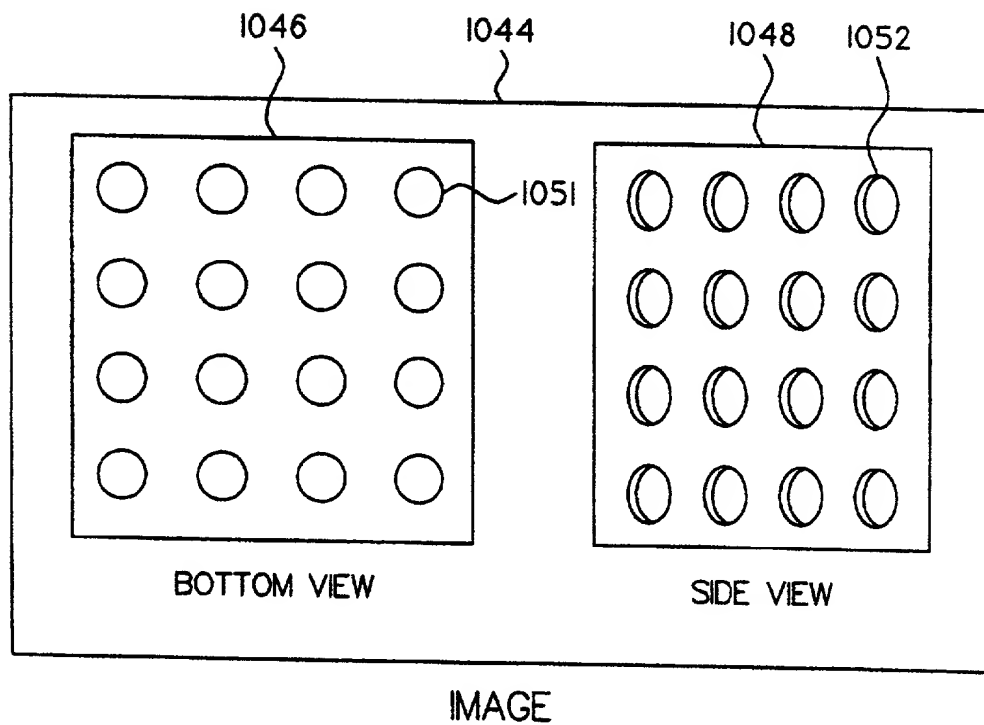


Fig. 18B